

1/20

FIG. 1
PRIOR ART

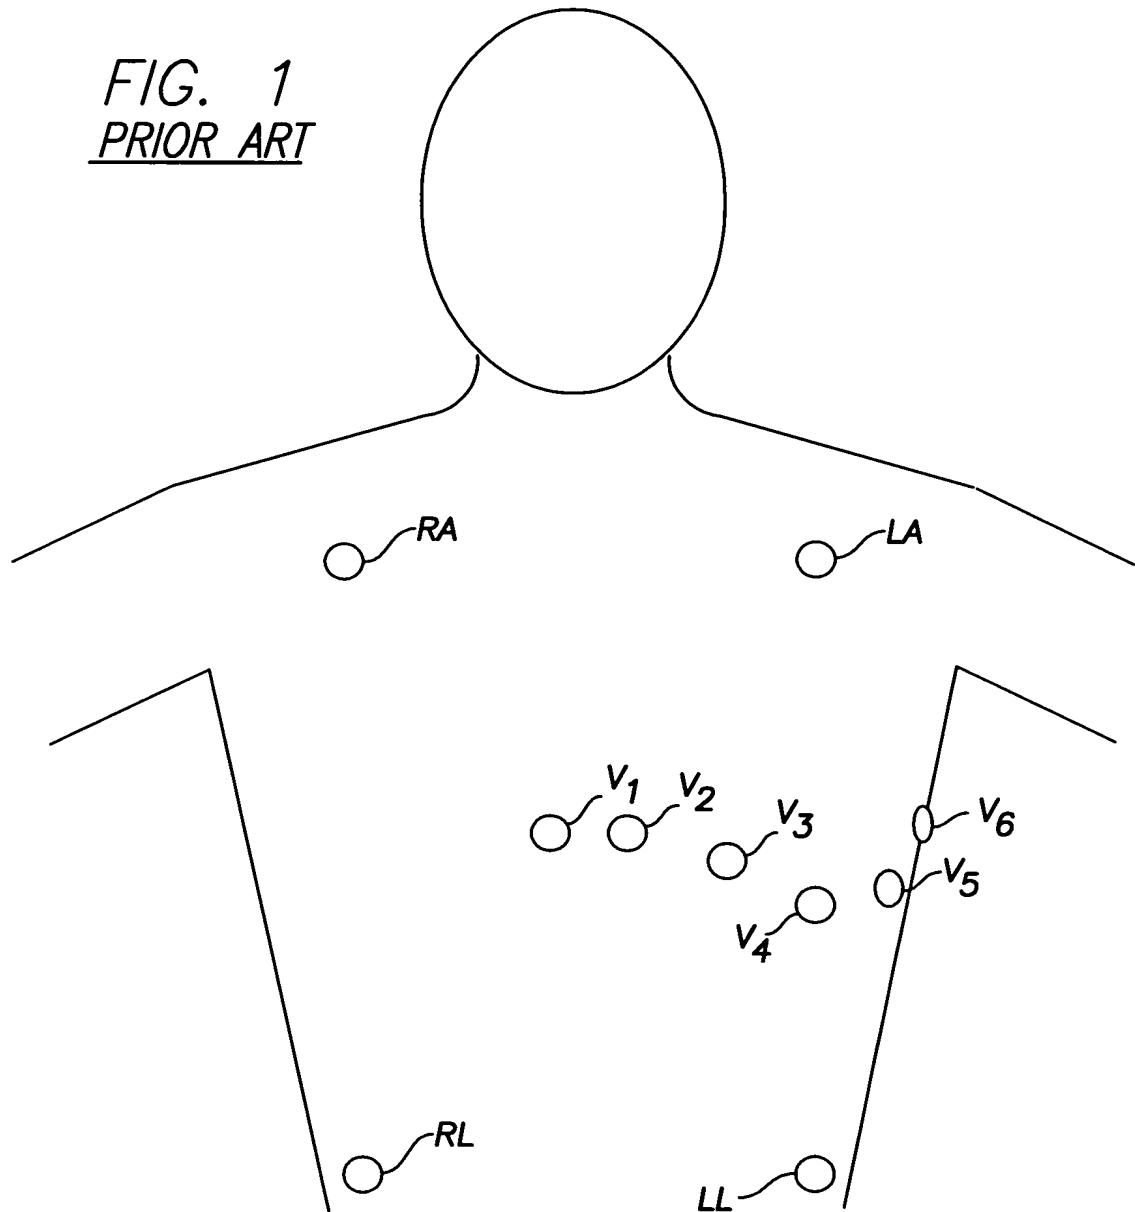
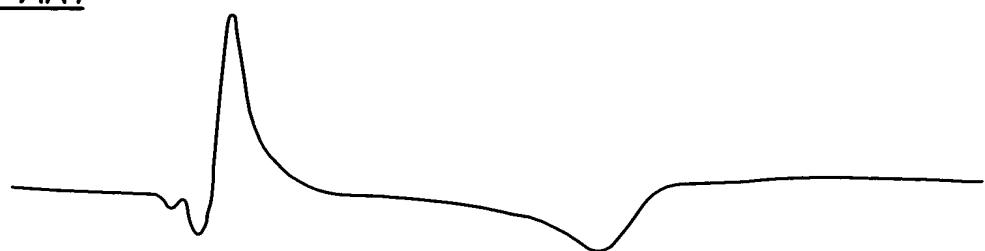
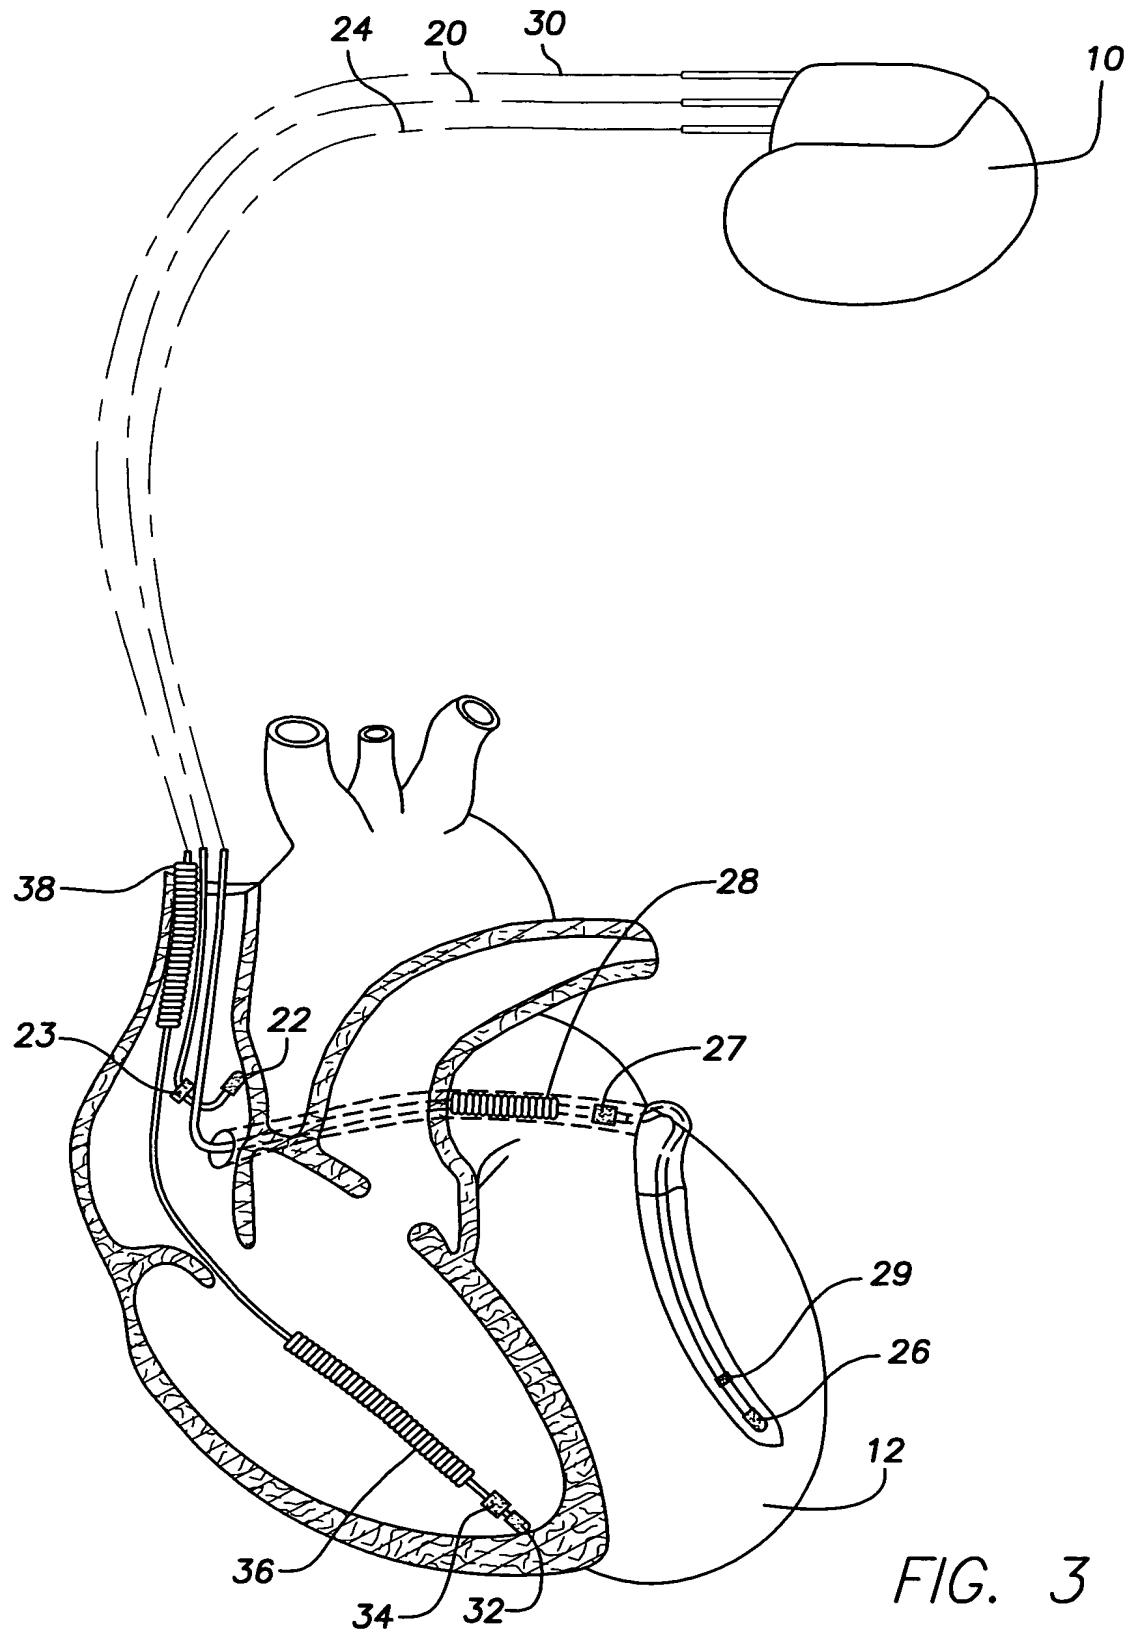


FIG. 2
PRIOR ART

COMBINED SURFACE EKG





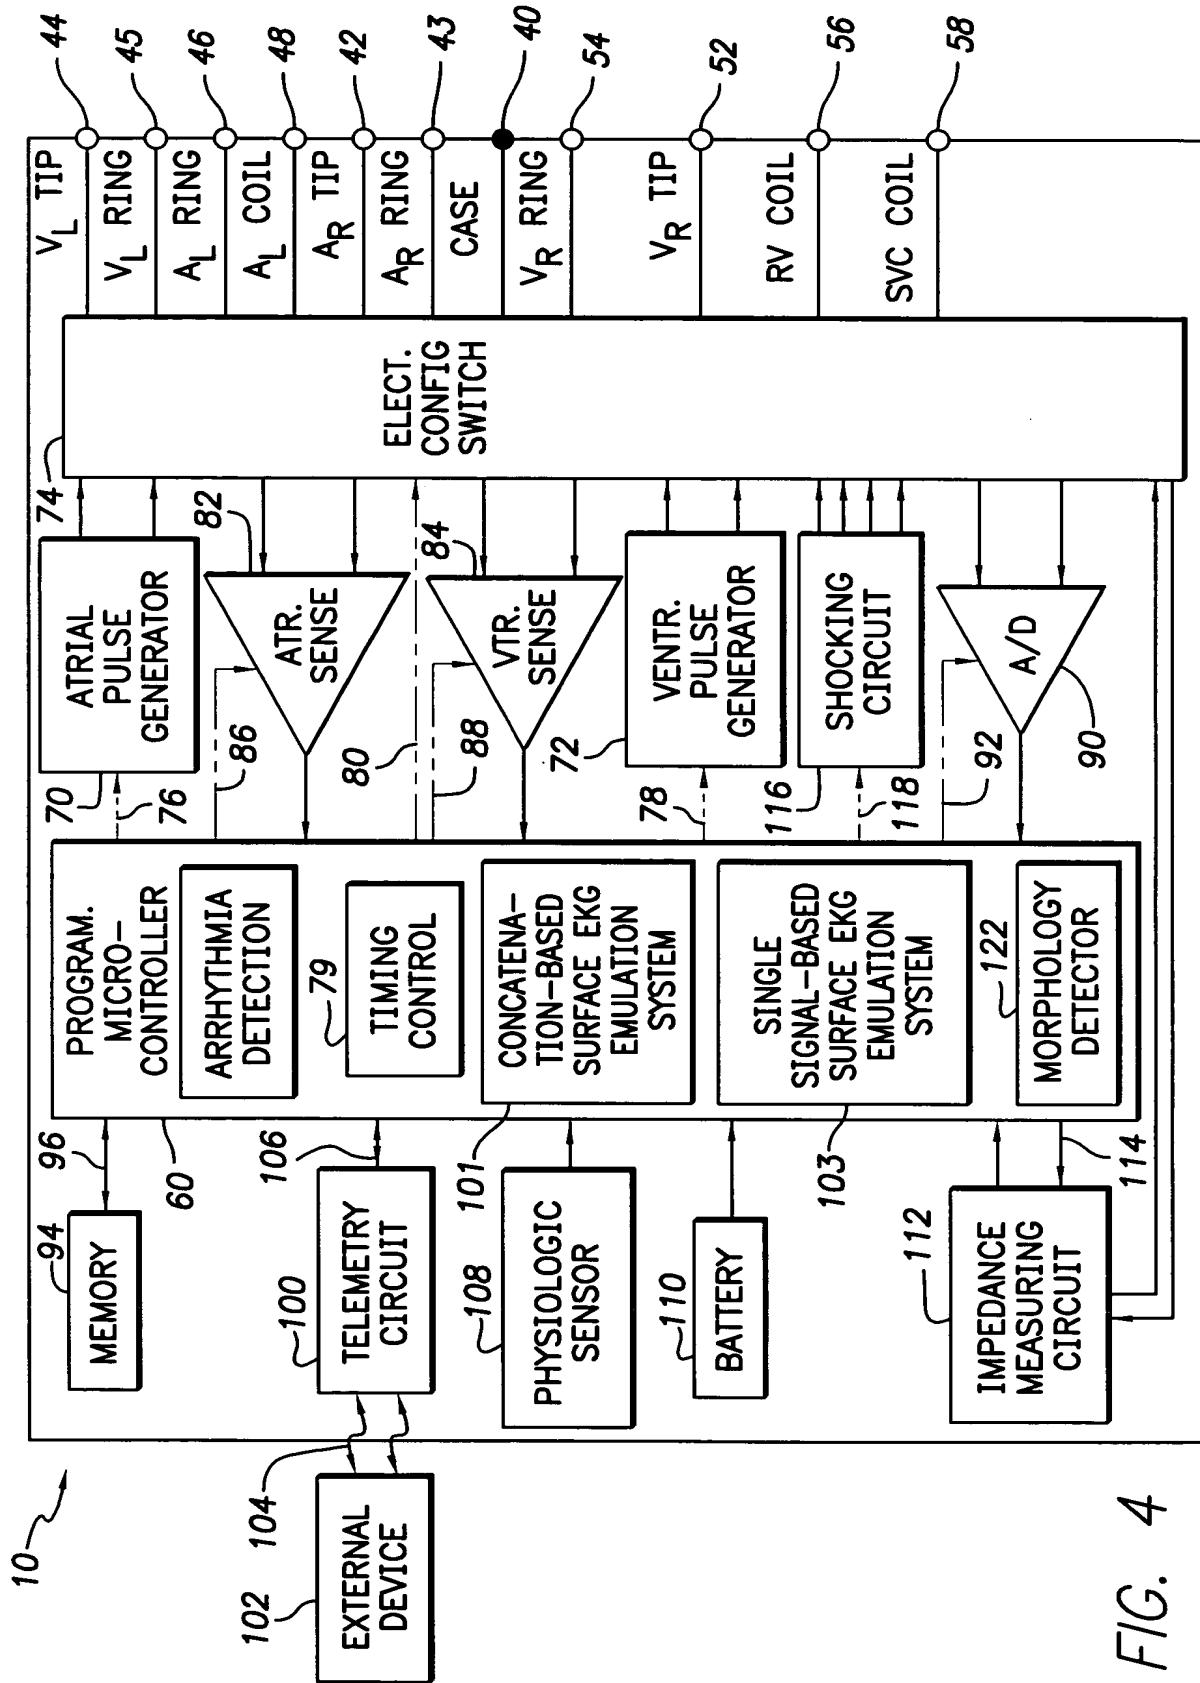


FIG. 4

FIG. 5

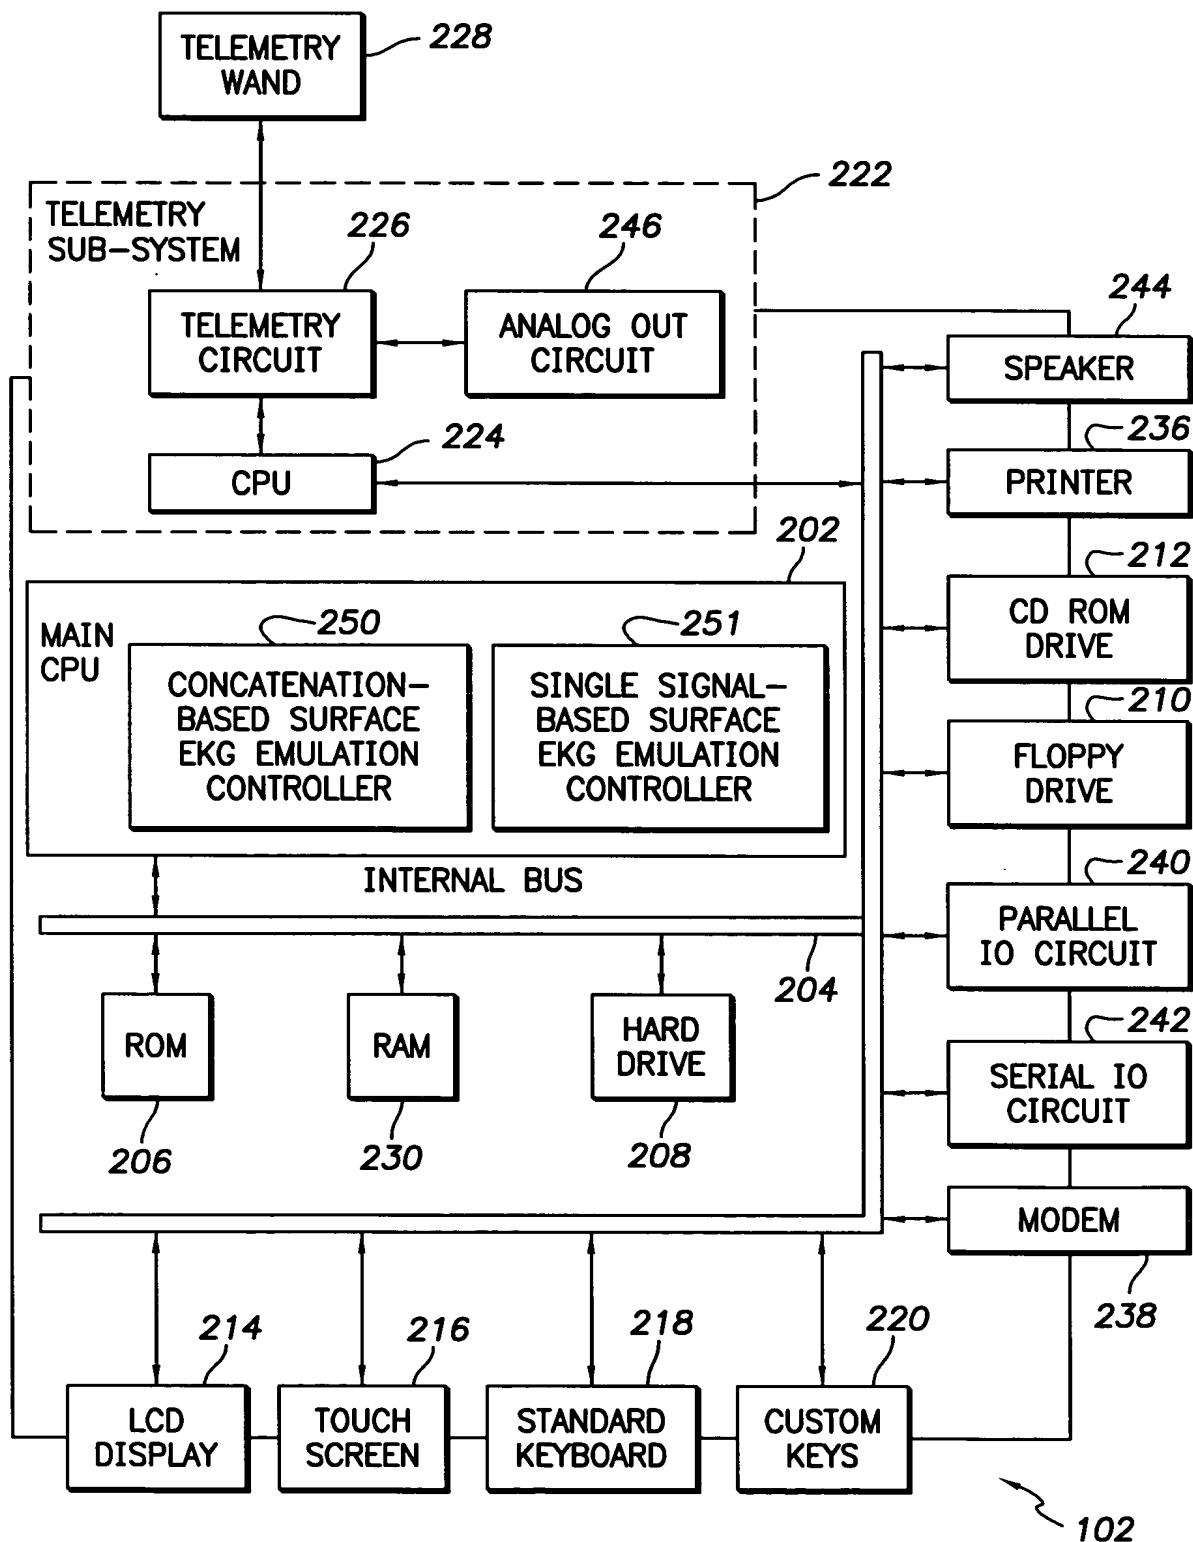


FIG. 6

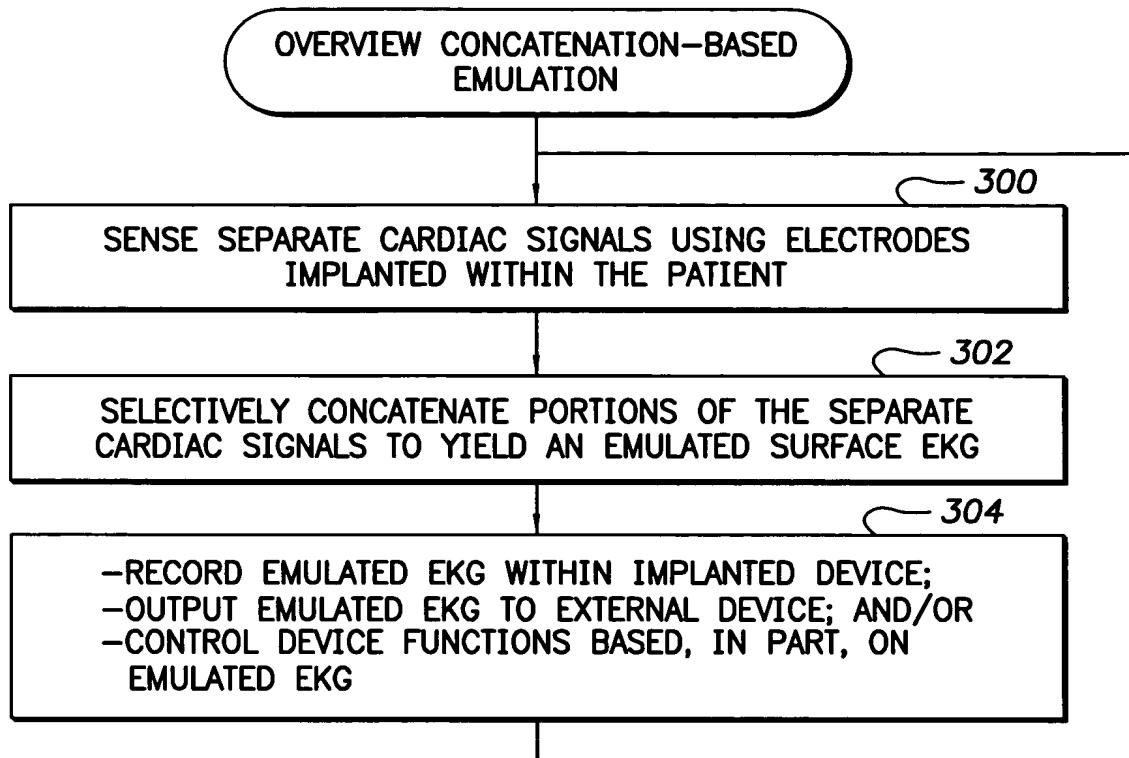


FIG. 7

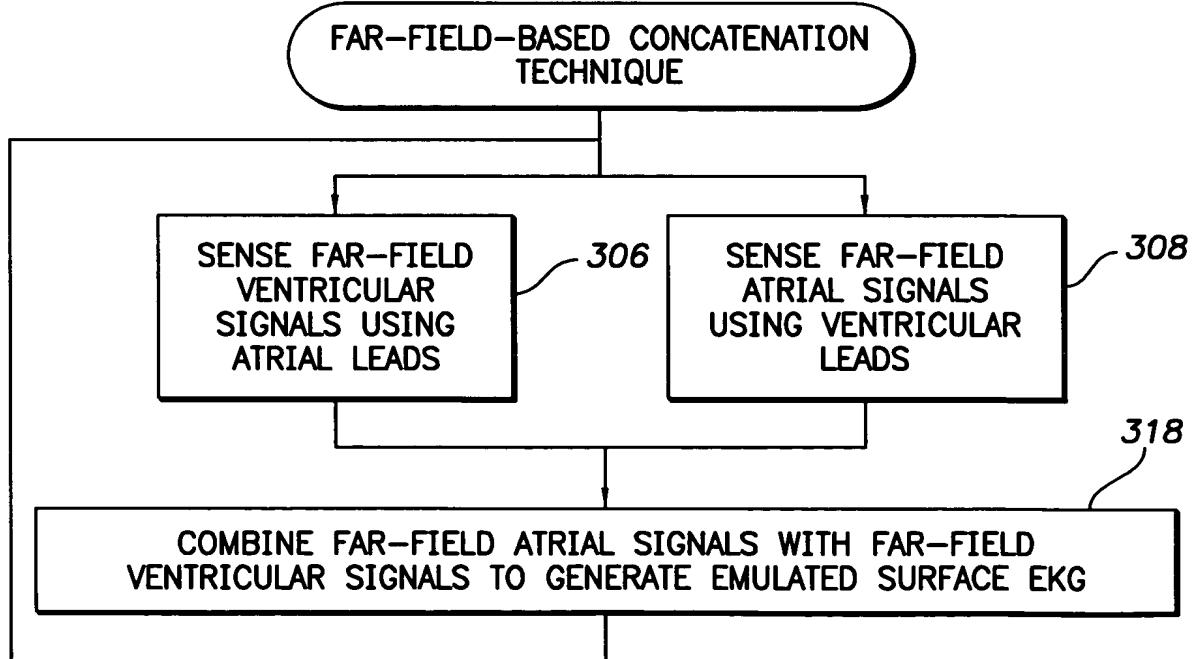


FIG. 8

FAR FIELD SENSING OF R AND T FROM ATRIAL CHANNEL




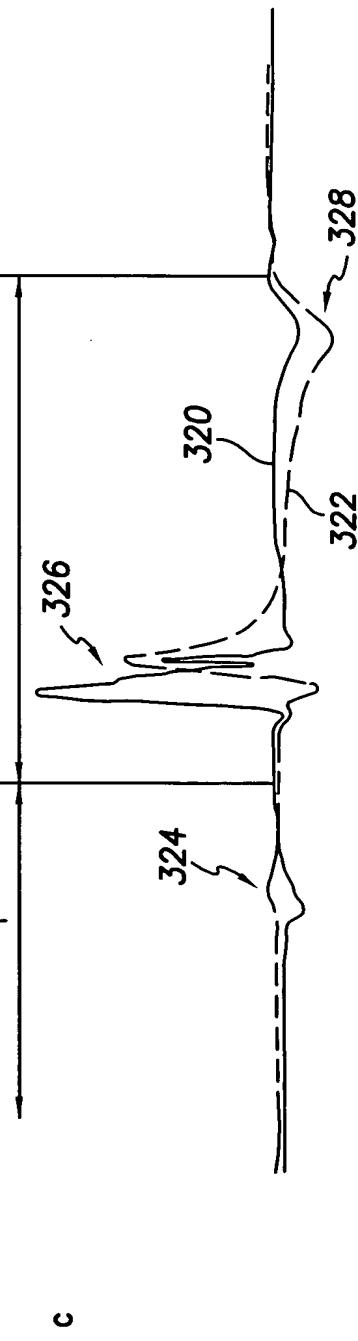


FIG. 9

7/20

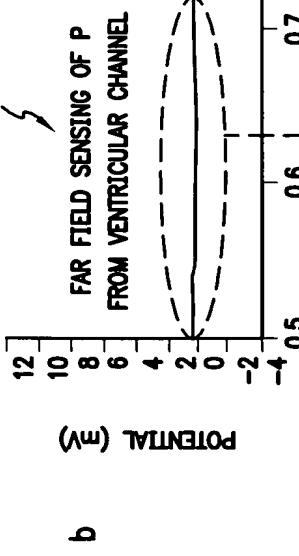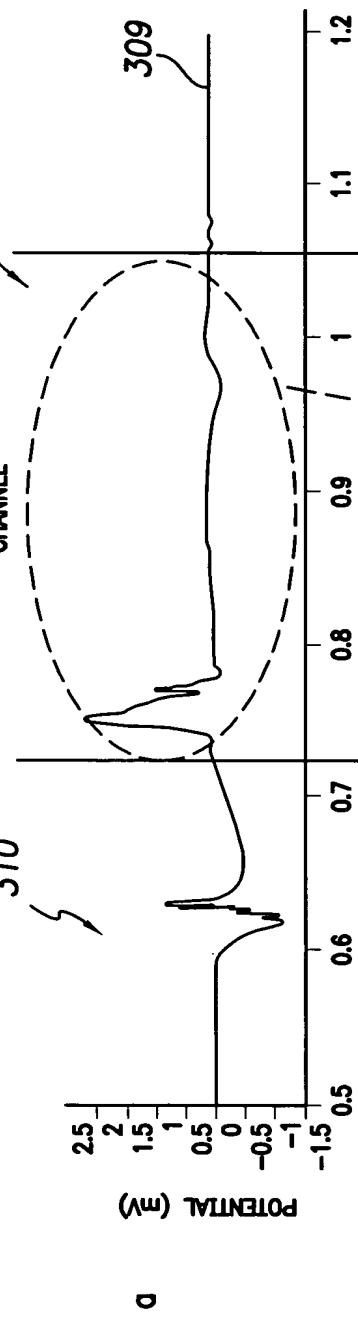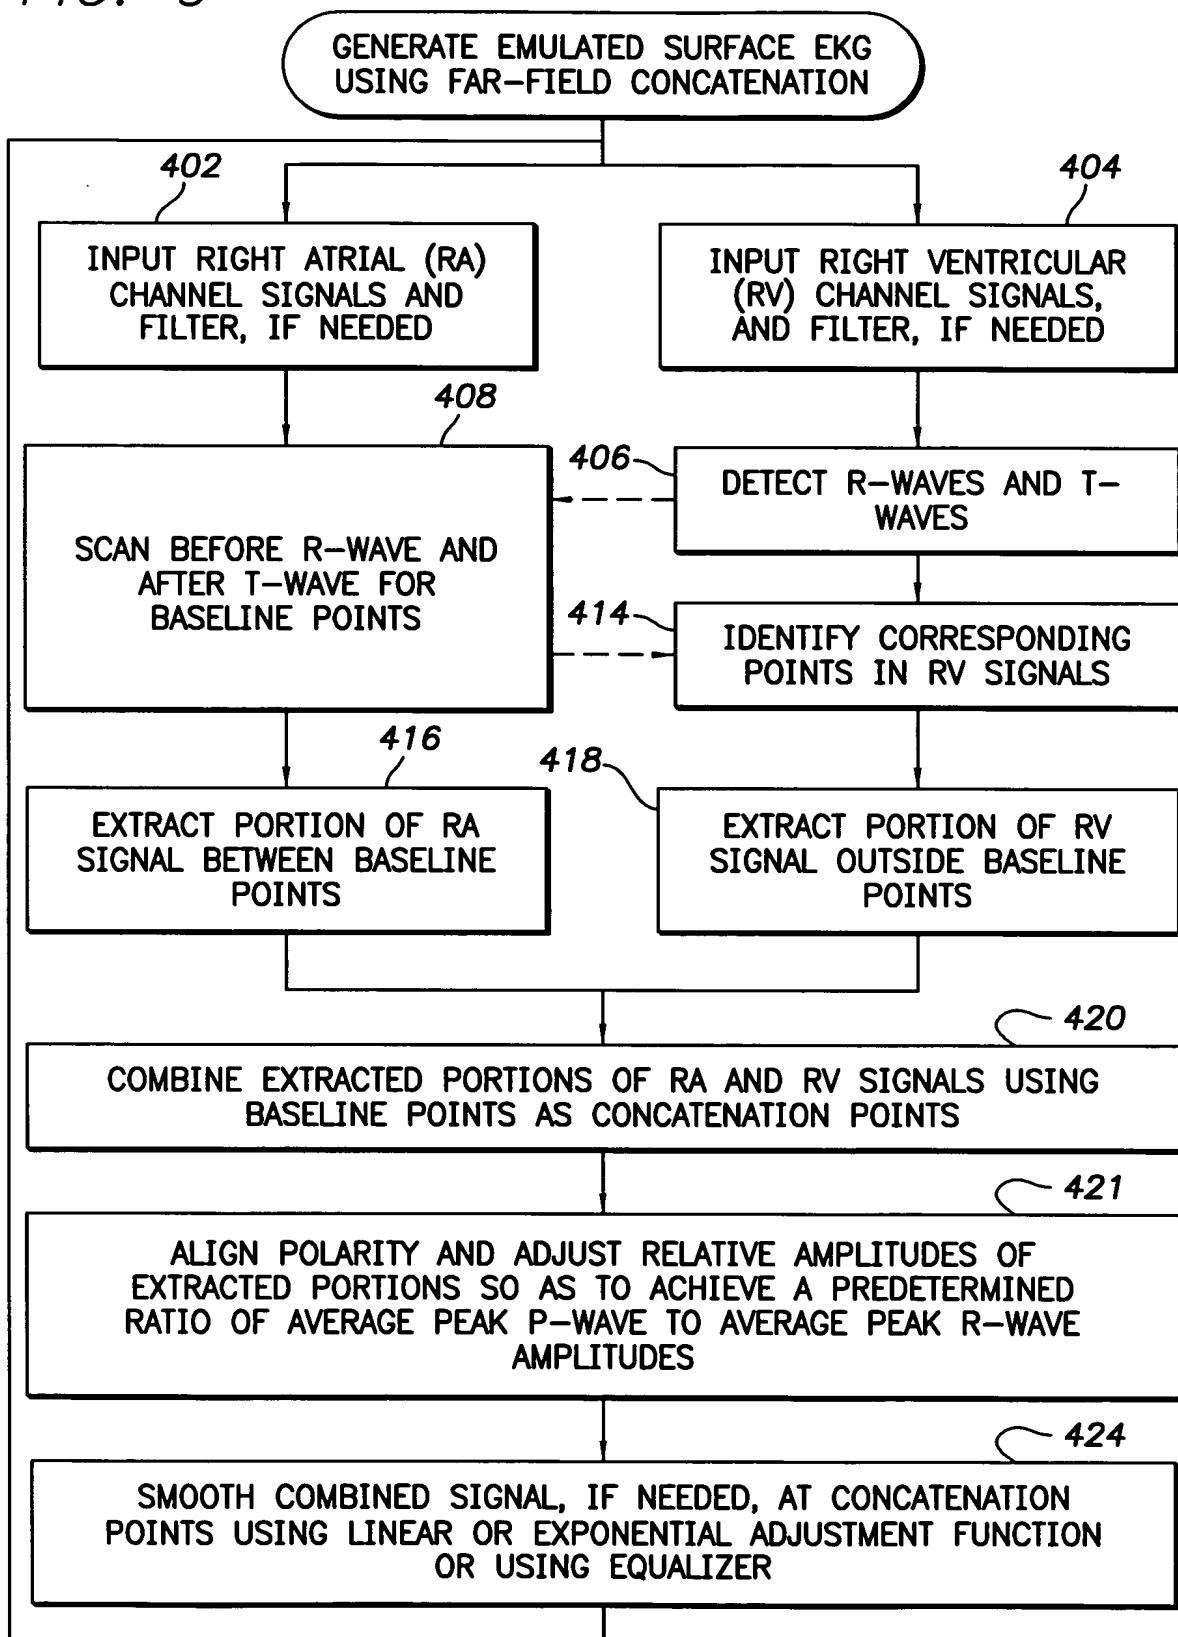

8/20

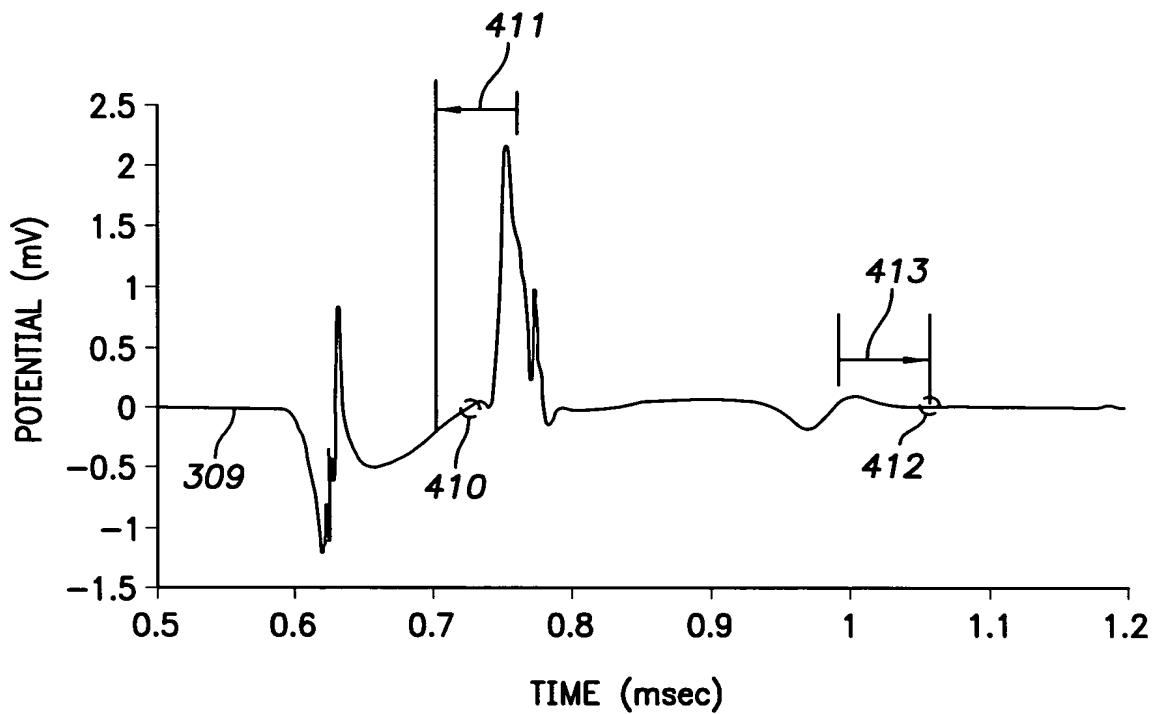


FIG. 10

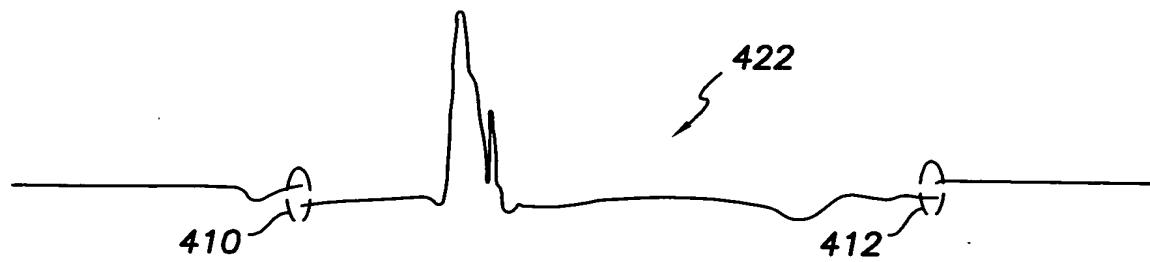


FIG. 11

9/20

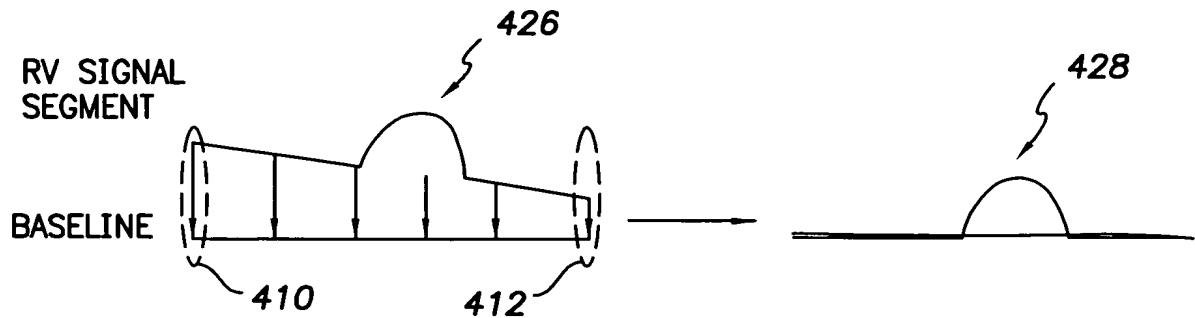


FIG. 12

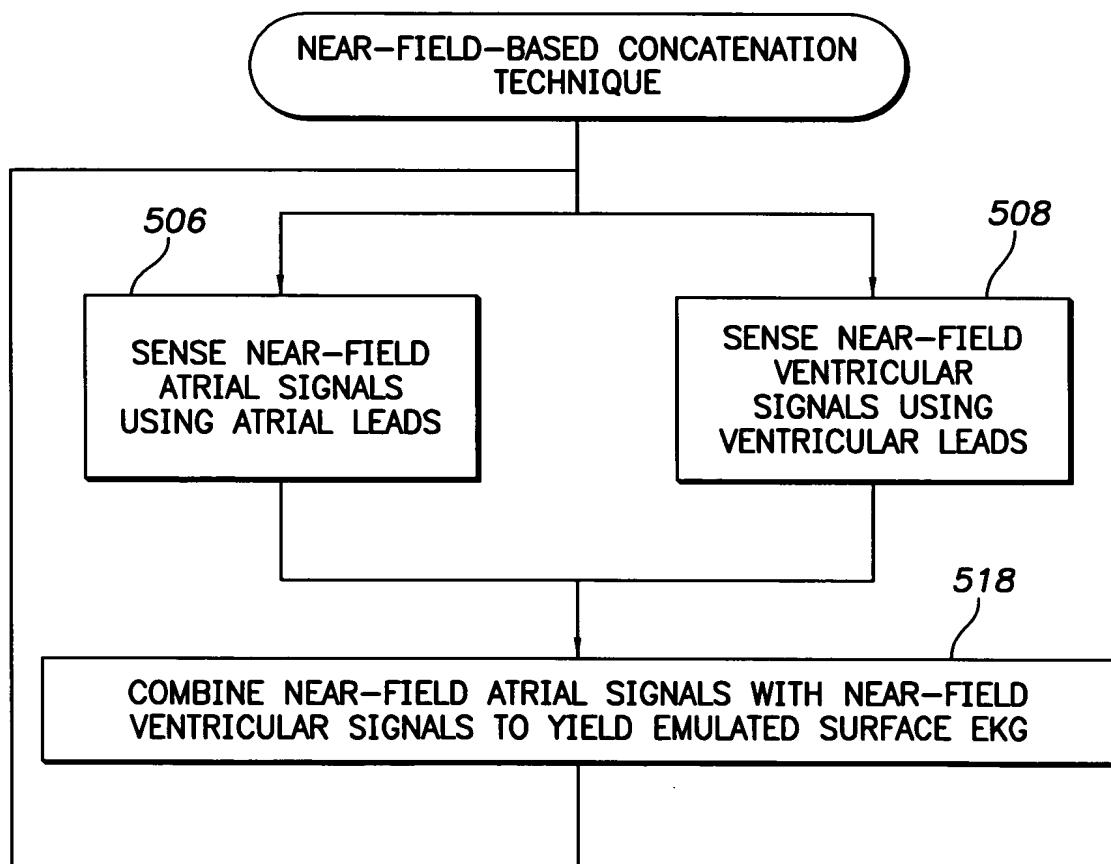


FIG. 13

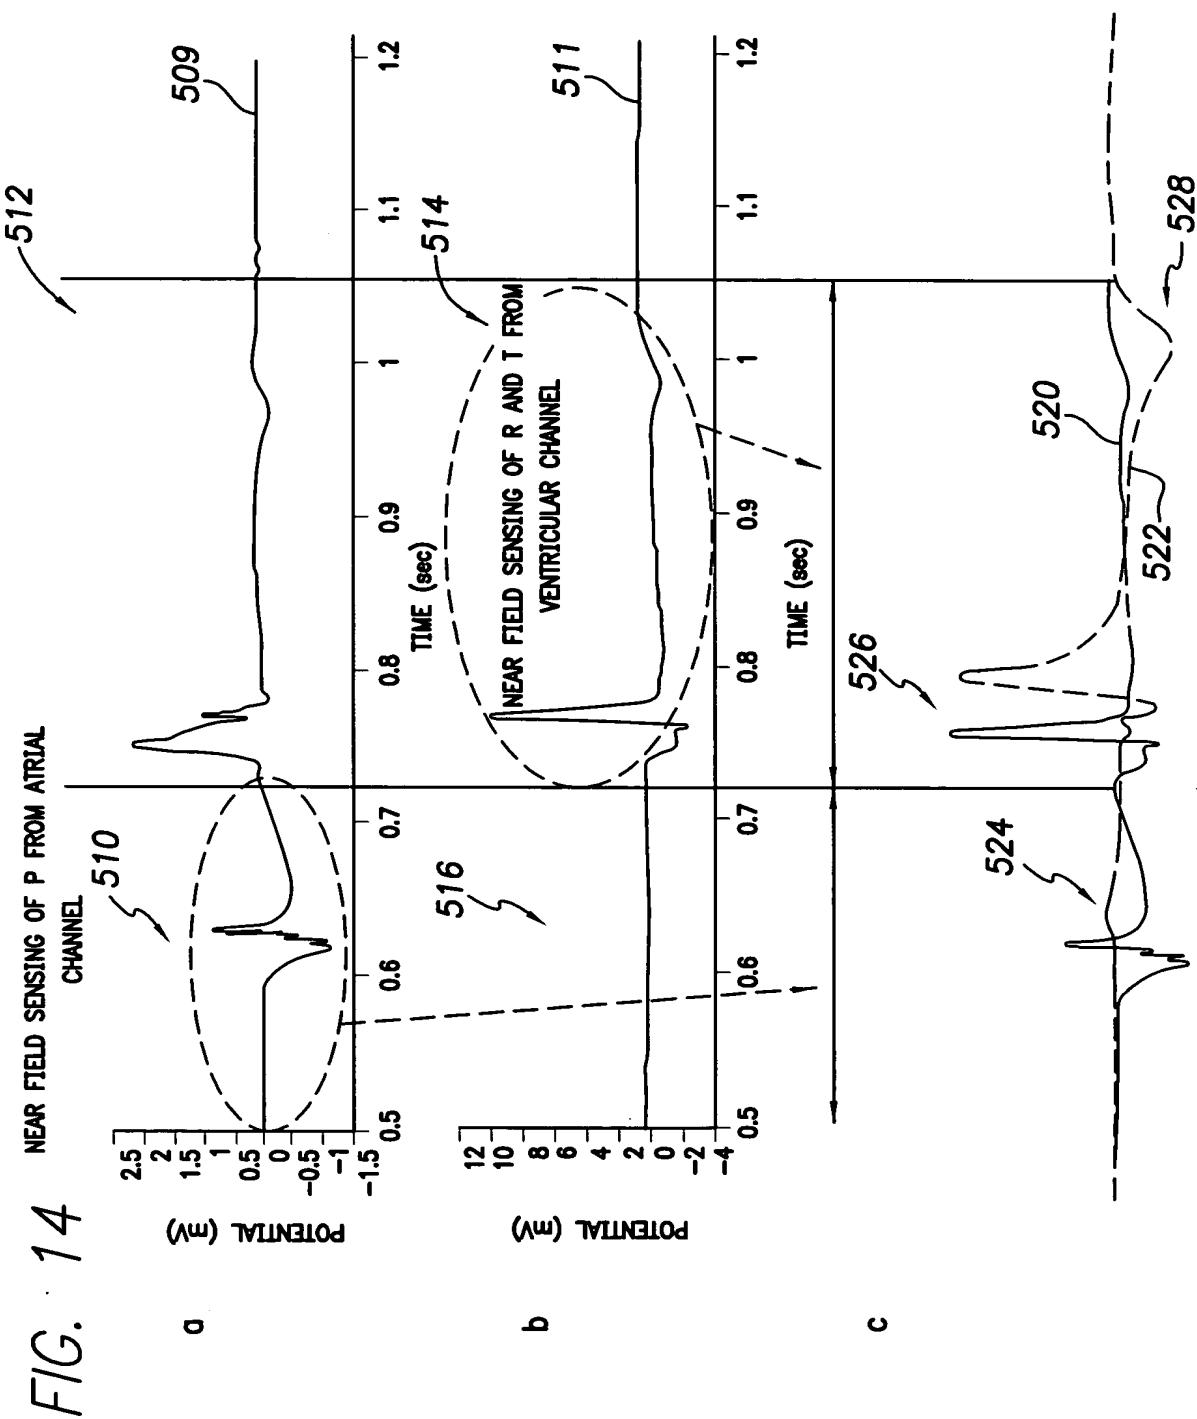
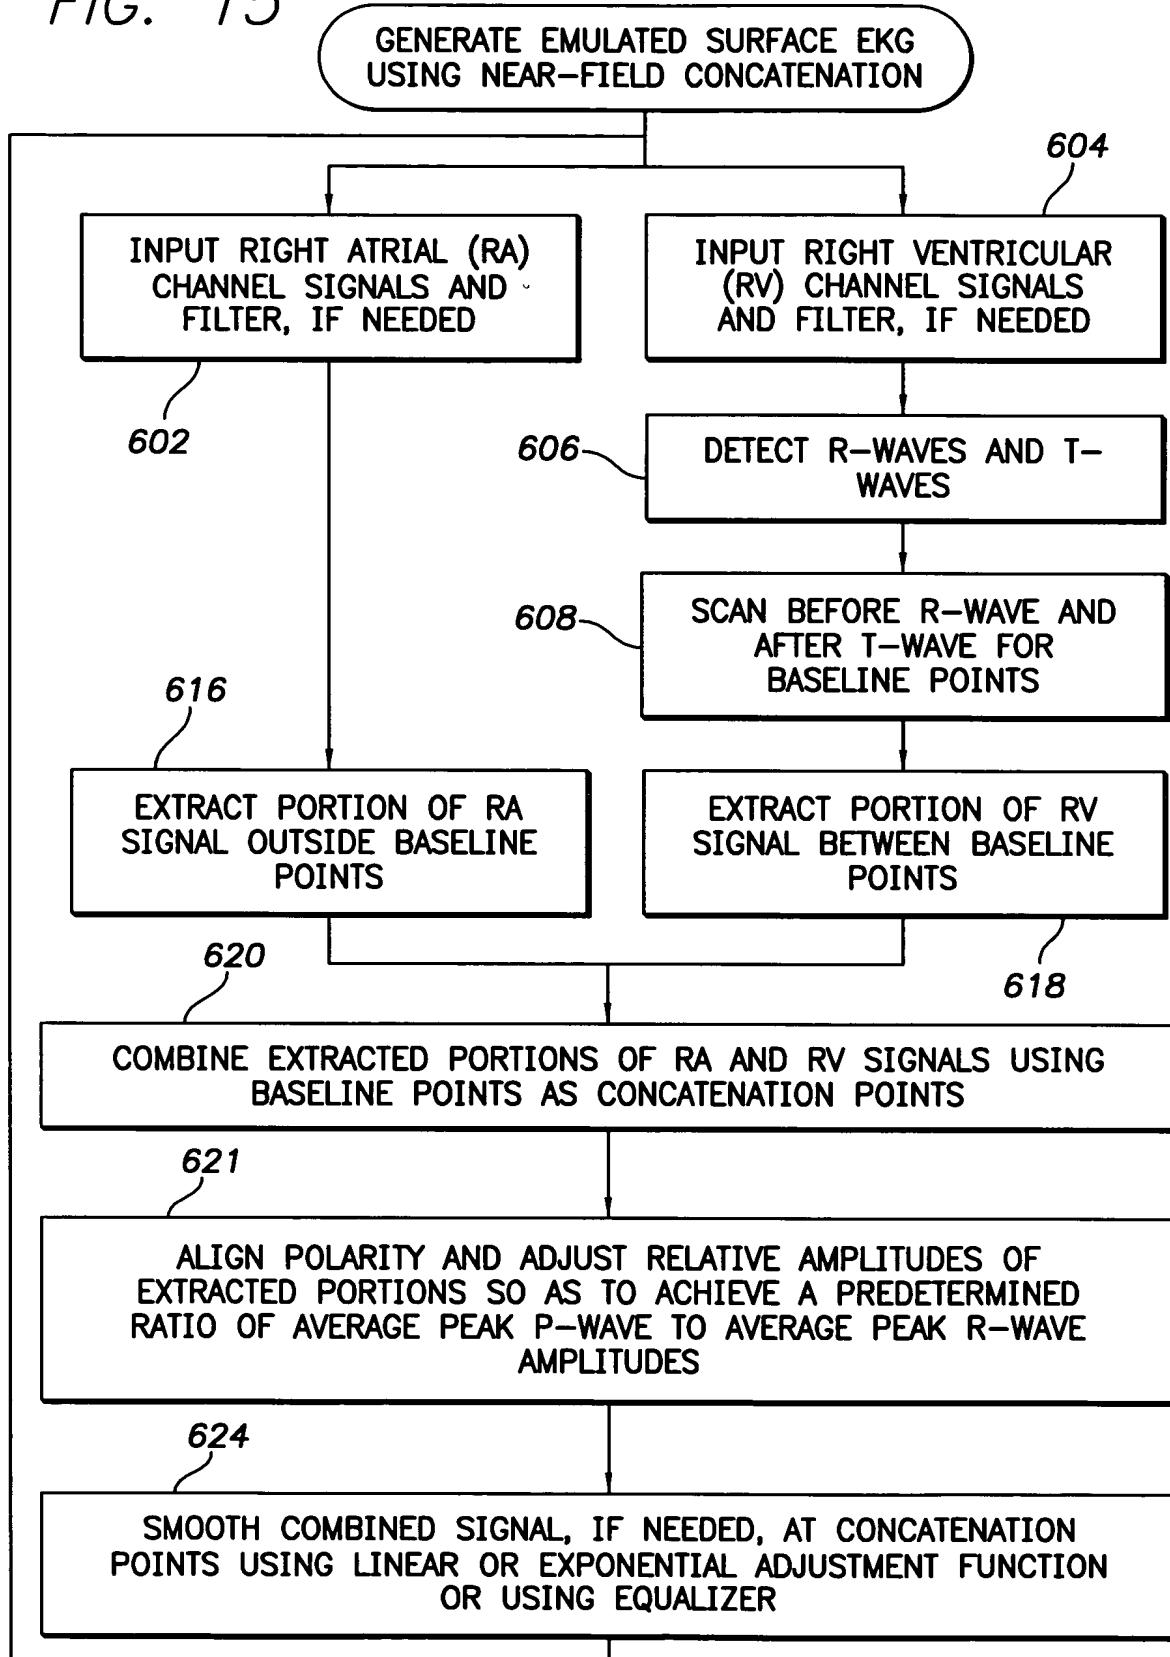


FIG. 15



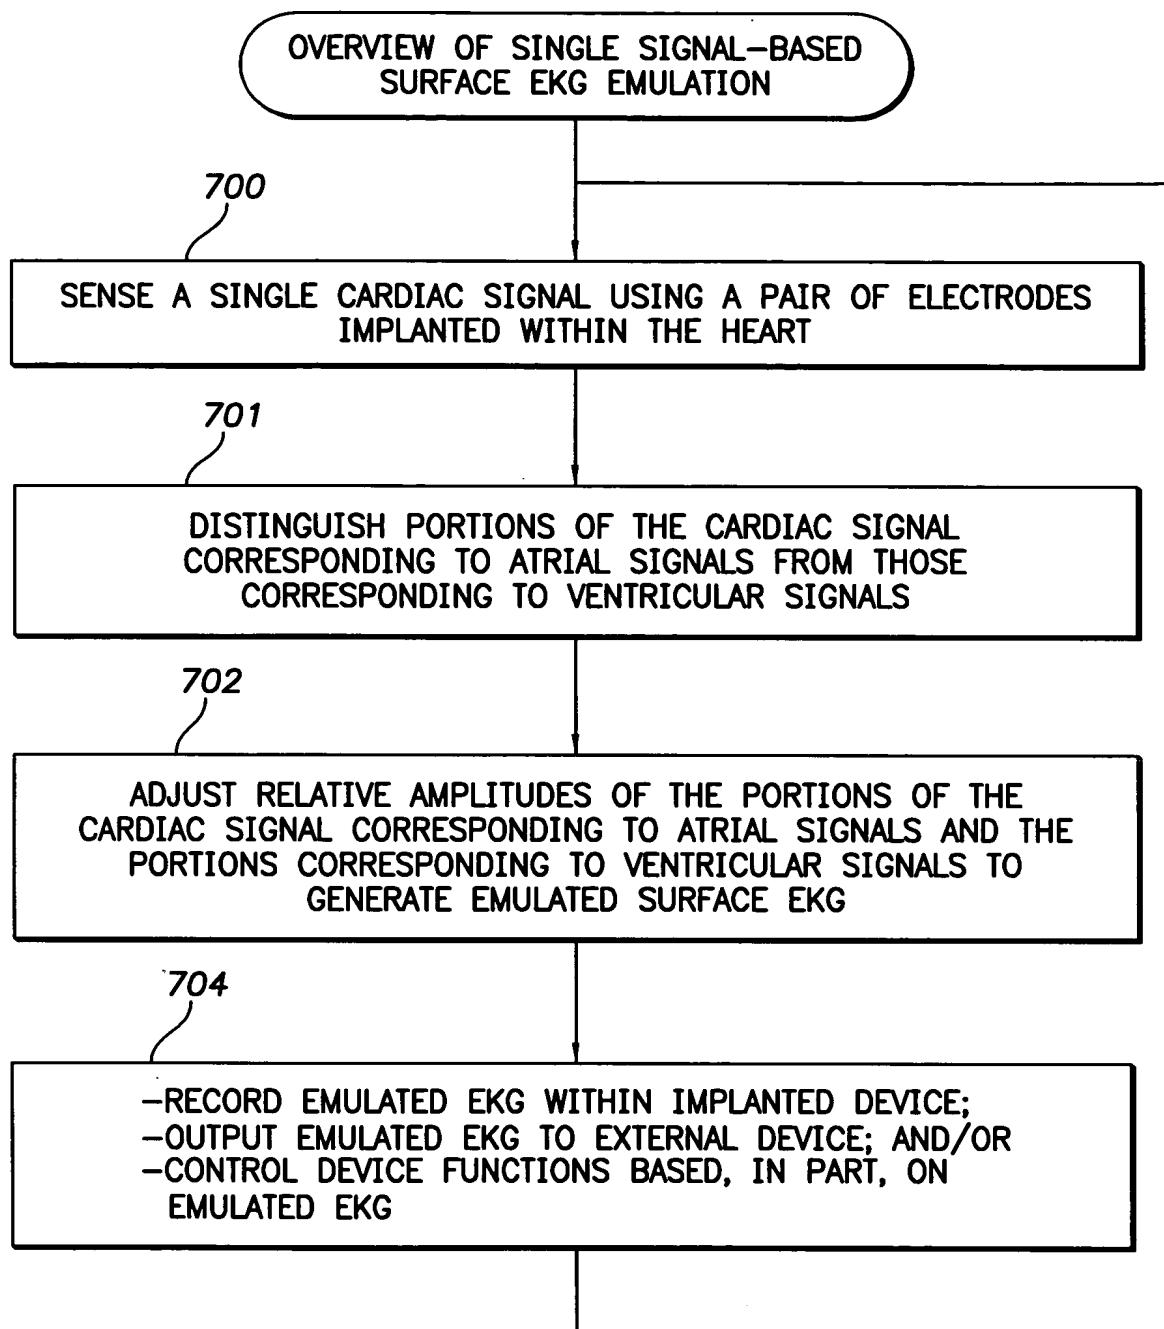


FIG. 16

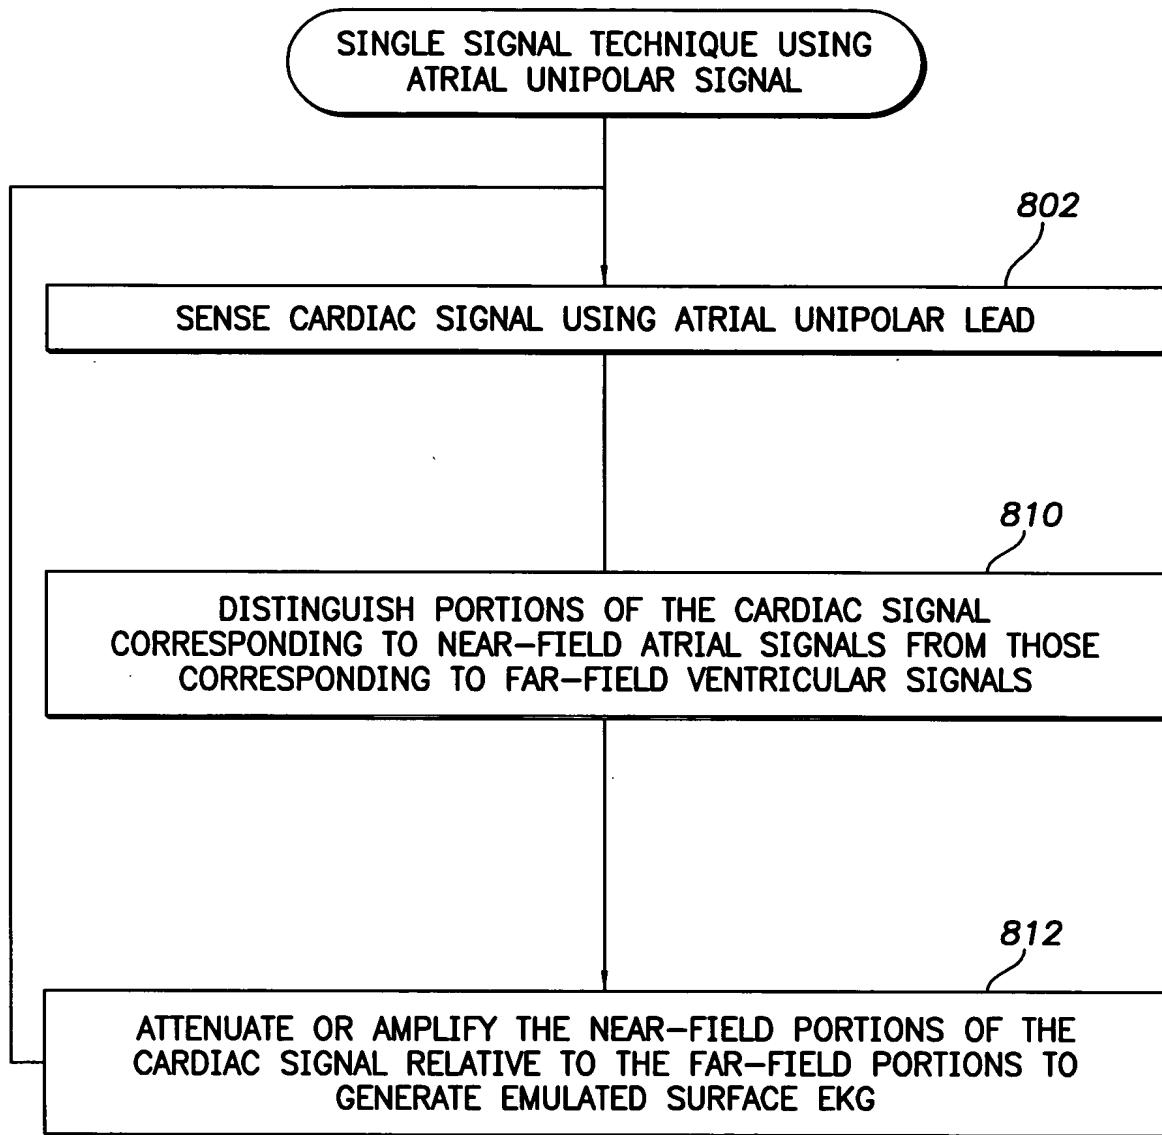
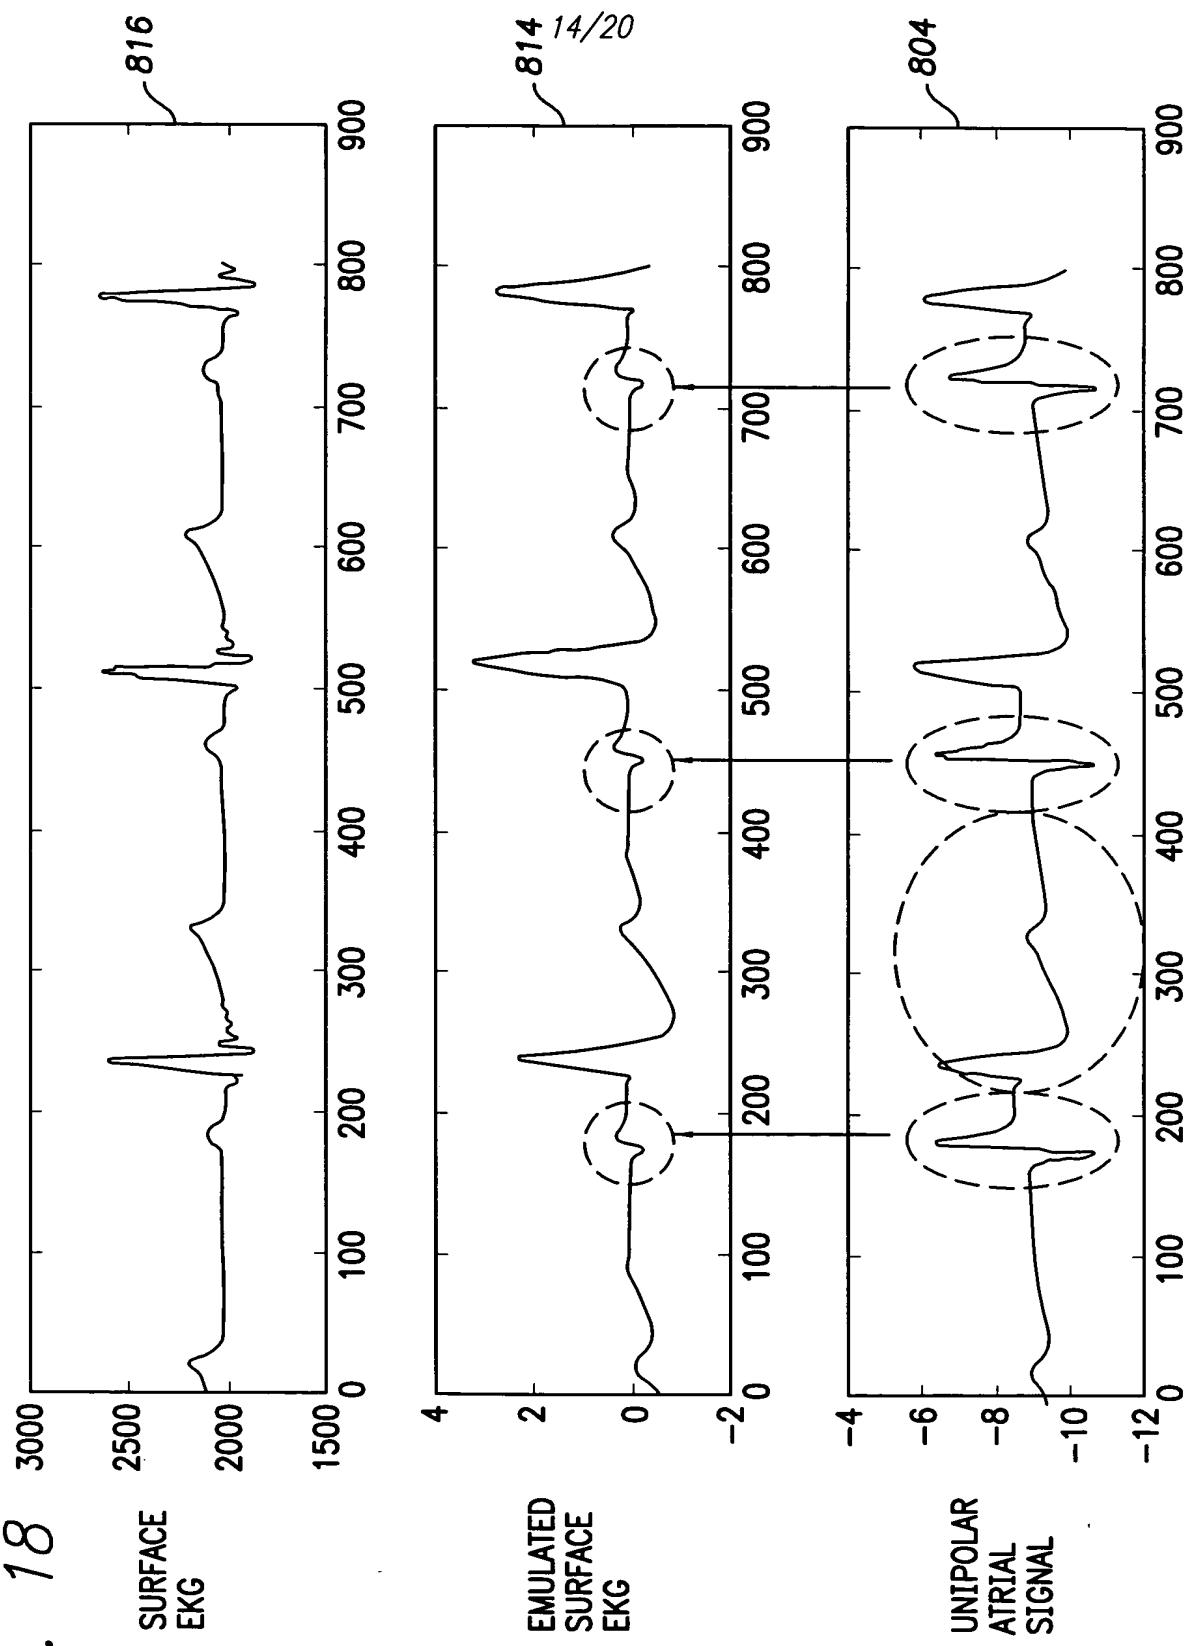


FIG. 17

FIG. 18



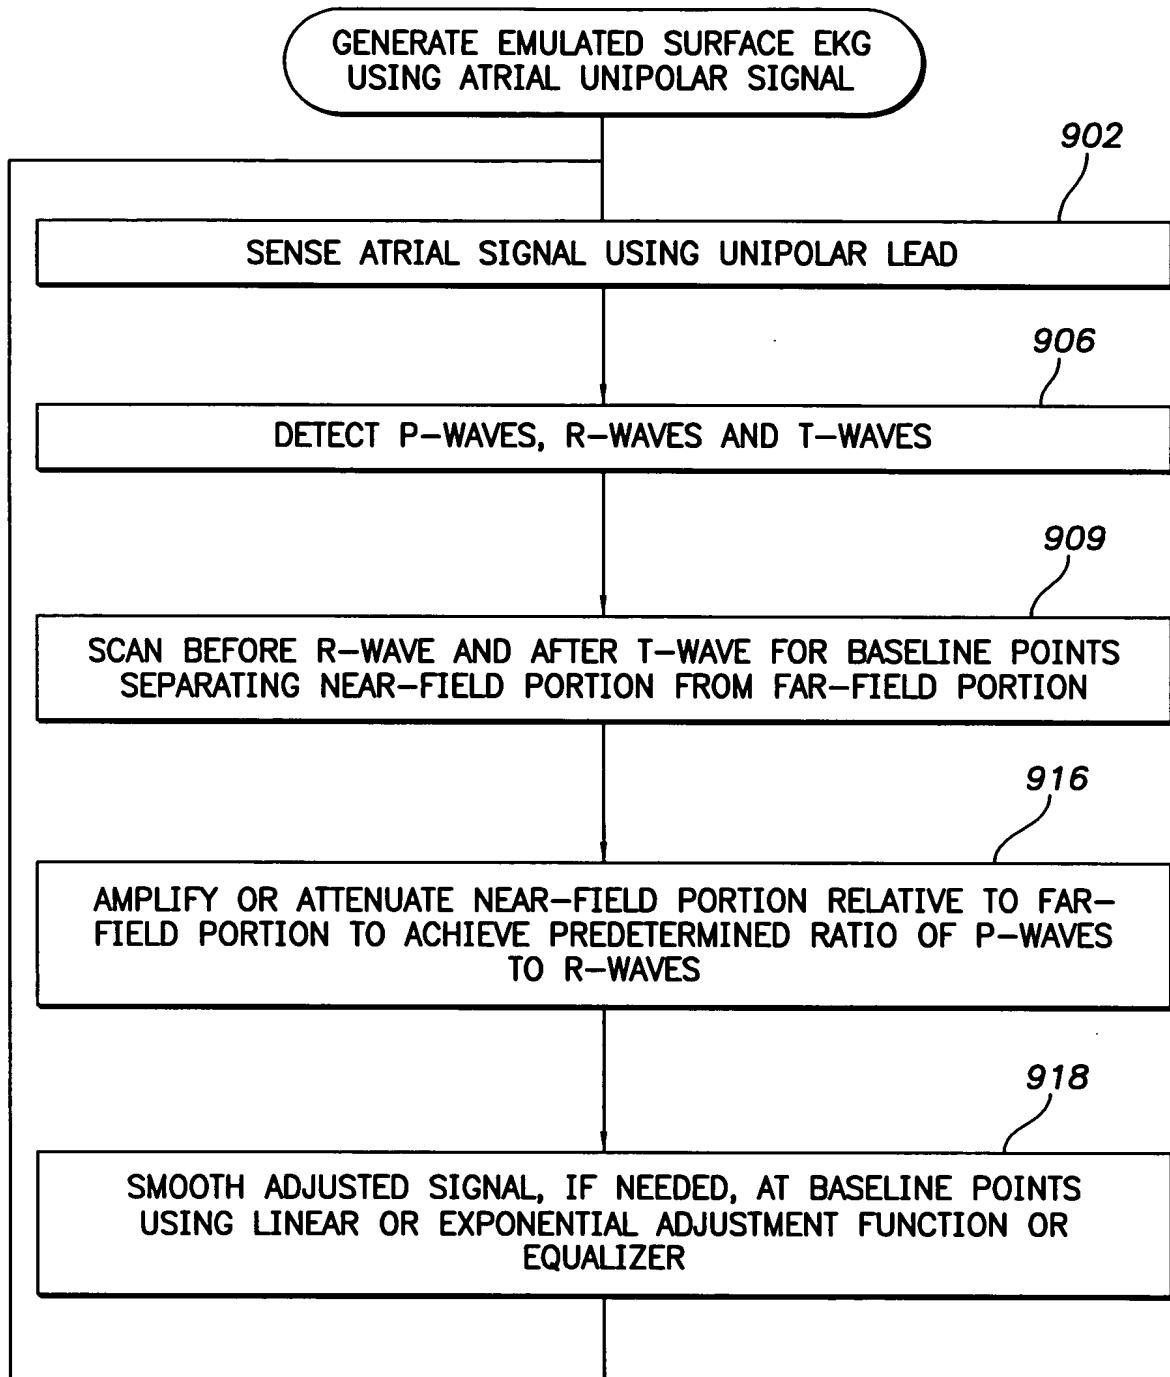


FIG. 19

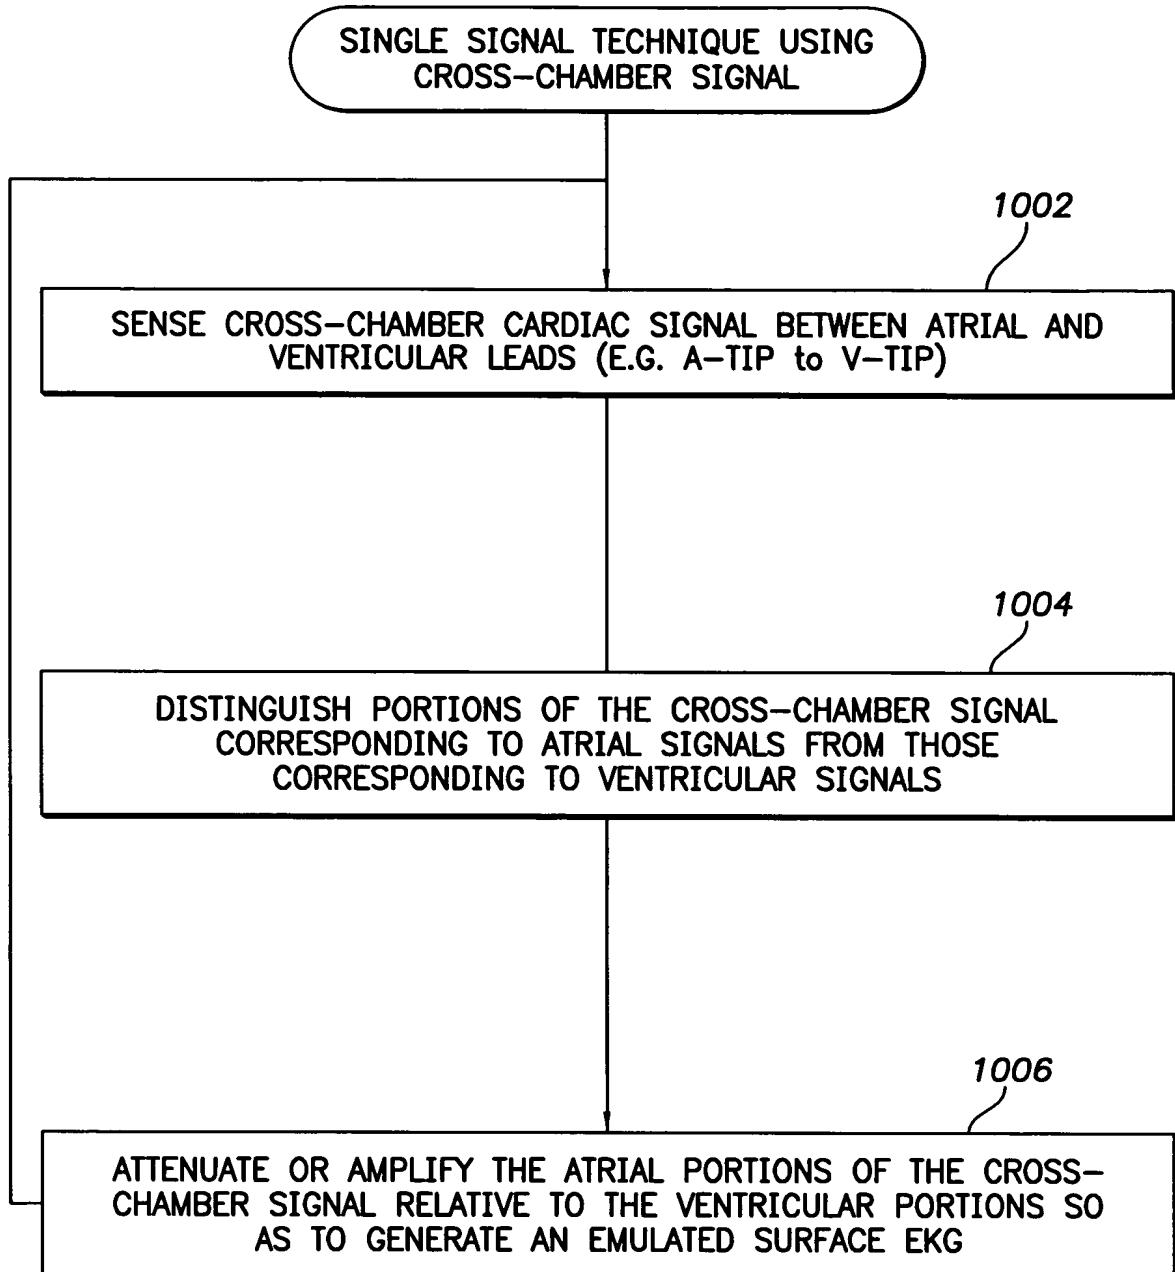


FIG. 20

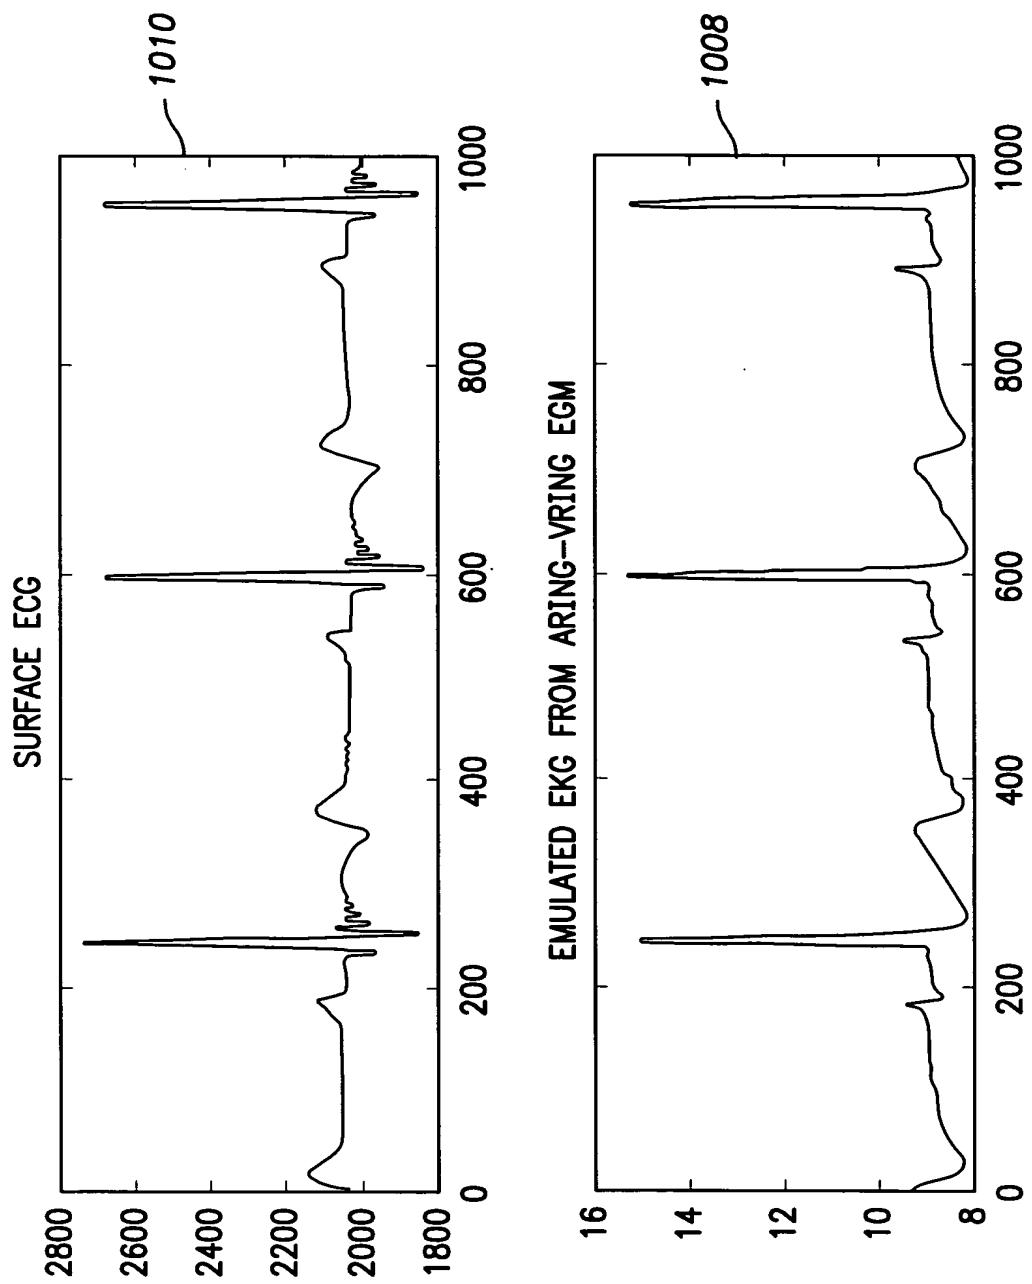


FIG. 21

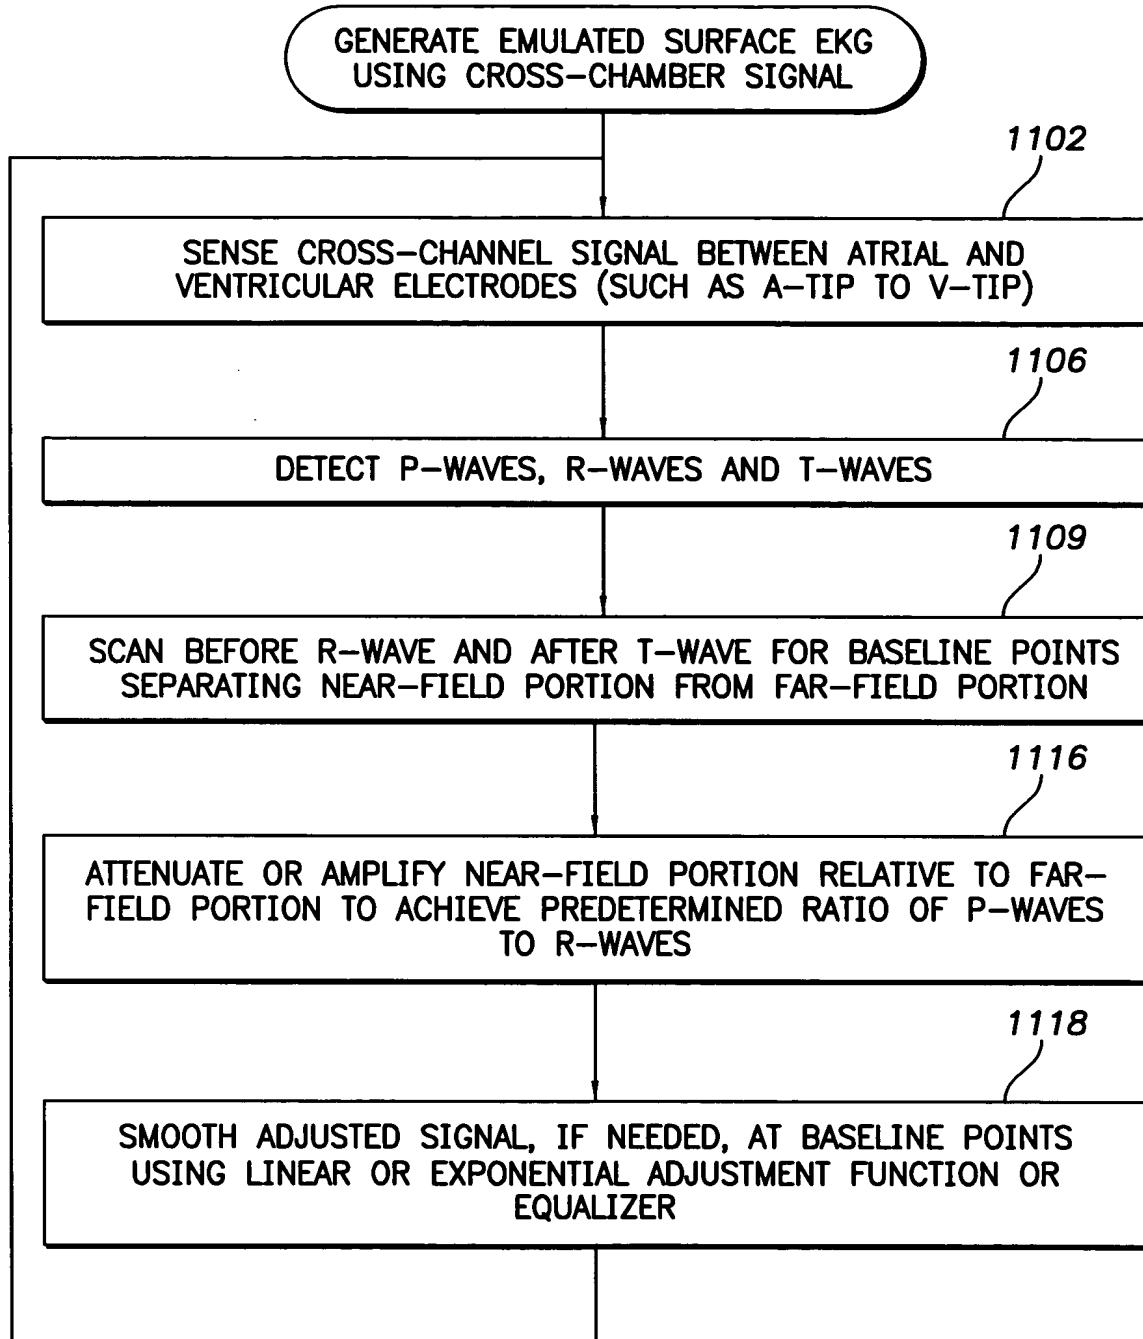


FIG. 22

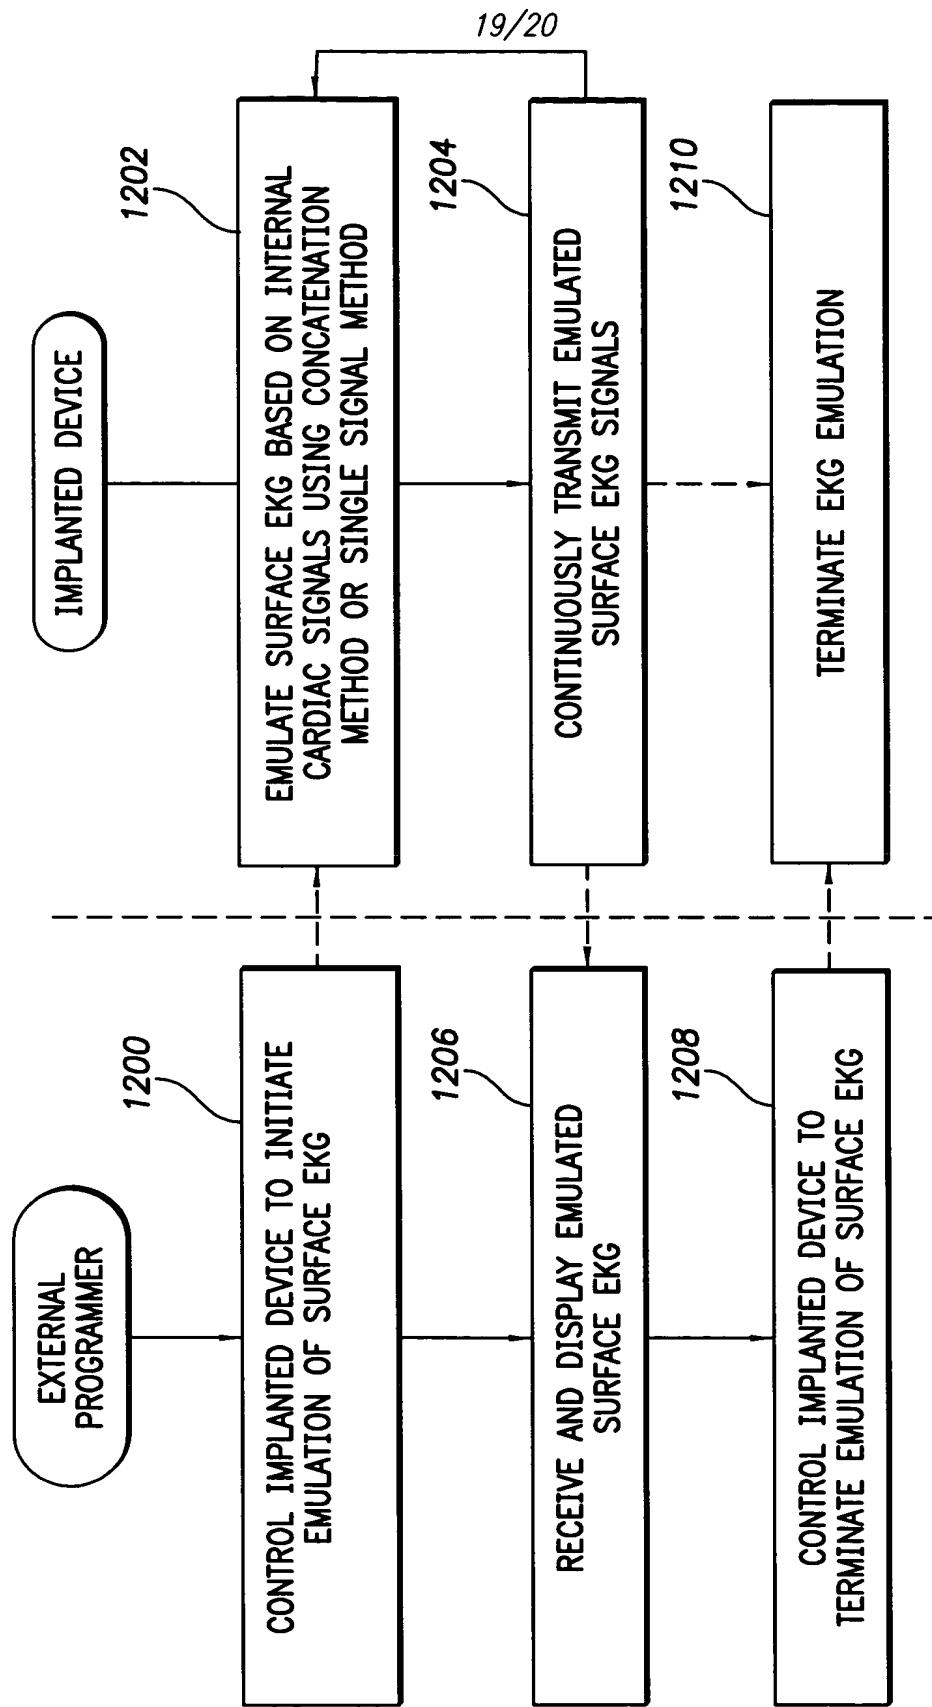


FIG. 23

FIG. 24

